

#### PRODUCT BROCHURE

# TREO®

Versatile by Design. Fit for any Anatomy.\*

\*Per IFU.





# Inspiring Confidence with Next-Generation Device Technology

Conversion to open repair through 3 years 1 (0/150)

Type III/IV Endoleak through 3 years 1 (0/150)


0%
Rupture through
3 years 1
(0/150)



#### **Fabric**

Woven Polyester with an optimized weave pattern

- ▶ Low profile
- High strength
- Low permeability



#### **Stents**

Electropolished Nitinol:

- Super-elastic properties
- Proven fatique endurance
- Suprarenal stent is laser-cut for durability



#### Suture

5-0 braided polyester surgical suture impregnated with PTFE

- High wear resistance
- ▶ High tensile strength



## Radiopaque Markers

- ▶ Platinum Iridium (90%-10%)
  - > Radiopaque material for enhanced visibility
  - > Low profile
  - > Galvanic corrosion resistance
- Positioned to aid device placement and easier contralateral gate cannulation

## The NEXT Evolution of EVAR is Here

The TREO® Abdominal Stent-Graft System is indicated for use in the endovascular treatment of patients with infrarenal abdominal aortic and aorto-iliac aneurysms with the following characteristics:

- Adequate iliac or femoral access compatible with the required delivery systems and accessories
- ▶ Minimum overall AAA treatment length (proximal landing location to distal landing location) of 13cm
- ▶ Minimum overall length from the lowest renal artery to the aortic bifurcation of 9cm

#### Proximal aortic landing zone with:

Infrarenal landing neck length of ≥15mm

Suprarenal neck angle of ≤ 45 degrees

Infrarenal neck angle of ≤ 60 degrees

Aortic neck diameters ≥17mm and ≤32mm

#### Distal iliac landing zone with:

An inside diameter of 8mm - 13mmand a length of  $\ge 10mm$ 

An inside diameter of >13mm - 20mm and a length of ≥15mm

100%
Technical Success (at index procedure)<sup>2</sup> (150/150)

100%
Freedom from aneurysm related mortality through 3 years 1 (150/150)



## TREO Key Features

#### Graft features

- Multiple size options
- ▶ Flexible graft design
- ▶ Dual active fixation

- Optimized proximal seal
- Lock stent technology



### Delivery system features

- Low profile delivery system
- Controlled, precise graft delivery
- Leave behind sheath
- Protective proximal clasp

## More Choices, More Possibilities

Multiple size options for planning and treatment versatility.

**90%** of procedures utilize 3 pieces <sup>2</sup>

True three-piece modular design with a wide variety of sizes, lengths and tapers


TRE0 offers

29,400
unique treatment options

Main Bodies

Cuff

Universal | 14mm Gates

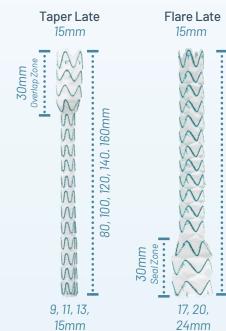


80, 100, 120, 140. 160mm

## Optimized Limb Tapering Design

- Limbs taper late in smaller diameters
- Limbs flare late in larger diameters
- ▶ In-situ adjustable limb landing zones

Resulting in expanded treatment options, particularly in tight/ narrow aortic bifurcations.

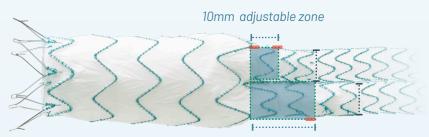


30mm adjustable zone

\*The use of the TREO stent graft also allows for in situ limb length flexibility. Both ipsilateral and contralateral gates have 1 to 3 cm of docking overlap, allowing for treatment of a more continuous range of patient anatomies and accurate targeting of the distal landing zone.\*\*

# Provides the Ideal Platform for Both Present and Future EVAR Needs

### Long main bodies provide:

- ▶ Lower displacement forces and increased endograft stability during the cardiac cycle 3,5
- ▶ Endograft closer to aortoiliac bifurcation makes it easier and faster to cannulate contralateral gate <sup>4</sup>

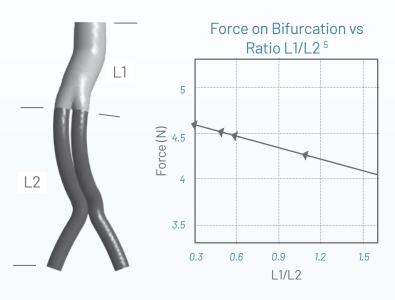






Ease of gate cannulation with long main body

TREO's long main body's ability to sit close to aortoiliac bifurcation, along with limb lock mechanism, may reduce the risk of both proximal and distal migration. <sup>5</sup>

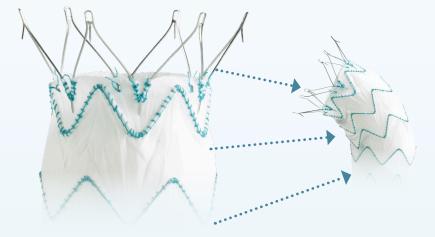


# Highly flexible design for challenging, angulated anatomy

- ▶ Z-Stent Configuration
- Space between stents

73% Of patients with hostile neck anatomy 8\* (27/37) 92%
Overall survival rate after 5 years 8\*

(34/37)

Freedrom from aortic related mortality through 5 years 8\* (37/37)





# Enhanced Proximal Fixation and Sealing: Optimal Outcomes


TREO is the only EVAR graft with both suprarenal and infrarenal active fixation and long, overlapping stents for an optimized proximal seal.

A SUPRARENAL & INFRARENAL FIXATION

 Two levels of fixation increase migration resistance.

#### IMPROVED PROXIMAL SEAL ZONE

Long overlapping proximal stents and seal stent sewn on the inside of graft pushes fabric against the aortic wall and increases vessel contact points for a confident seal and low type 1a endoleak rate.

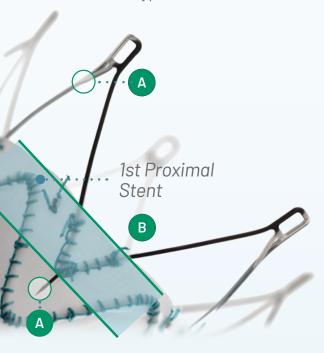

**0.8%**Type 1a endoleak at 1 year 1 (1/144)

0%
Migration through
3 years 1
(0/150)



## Overlapped Proximal End Configuration

▶ 3 seal points per apex

20mm-28mm Diameters 30mm-36mm Diameters

5 Peak Design = 15 seal points

6 Peak Design = 18 seal points









"Infrarenal barbs provide additional fixation and contribute to migration resistance in large, angulated necks." 4

Images provided courtesy of Neal Cayne, MD

# Unique Limb Lock Stent Technology

Designed to prevent limb disconnection and Type III endoleaks.

#### Rounded Barbs

inside main body gates are designed to securely engage with limb stents. The lock stent barbs are dulled to ensure compatibility with balloons.<sup>10</sup>

# Lock Stent Technology increases pull out force resistance by **6 times** <sup>11</sup>





Type III endoleak through 3 years 1 (0/150)





Example: Type III/DisconnectionEL 12

"Dual active proximal fixation and rounded barbs at the limb docking sites have been shown to multiply the migration and detachment pullout forces and might mitigate the development of Type I and III endoleaks respectively."

# Intuitive Mechanical Advantage for Controlled and Precise Device Deployment

A Low-Profile delivery system & Leave Behind Sheath are designed to enable percutaneous access and fewer sheath exchanges, facilitating a reduction in:


- Access Vessel Trauma and complications 13,14
- ▶ Procedural time, hospital length of stay and cost <sup>13,14</sup>
- ▶ Patient post-operative pain 14



# 1 INTRODUCER AND LEAVE BEHIND SHEATH

▶ Low profile introducer and detachable, leave-behind sheath (18/19 Fr OD) with hydrophilic coating and Flexible tip for easier navigation

Bi-directional flush port



## 2 PROXIMAL CLASPING

 Proximal clasp allows for safe graft re-positioning and delivery system removal

## 3 PRECISE DELIVERY SYSTEM

▶ The mechanical deployment provides controlled and stable stent-graft deployment


## 4 PROXIMAL CLASP RELEASE








Main Body De	elivery System	Leg Extension Delivery System		
20 - 28mm	30 - 36mm	9 - 15mm	17 - 24mm	
18Fr(OD)	19Fr(OD)	13Fr(OD)	14Fr(OD)	
		••••		




Highly visible proximal markers allow accurate alignment with lowest renal artery




\*\*The device may be repositioned until the proximal clasp is released reducing the risk of proximal misdeployment and improving the accuracy of landing the device below the renal arteries \*\* 10

# Optimized Design for Patient Safety and Procedural Success

Proximal clasp allows for safe graft re-positioning and delivery system removal.

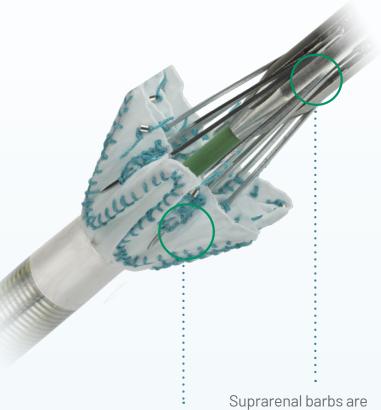

Infrarenal barbs are obscured in graft fabric "valleys" prior to final clasp release Suprarenal barbs are completely covered allowing graft to be safely repositioned until clasp is released

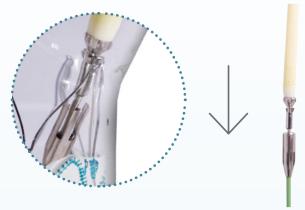

Proximal Clasp Simple Caudal Removal

Easily withdraw delivery system without added steps or risk of entanglement

 Proximal clasp prevents barb engagement with vessel wall until released

100%
Technical Success <sup>2</sup>
(at index procedure; 150/150)

Conversions to open repair through 3 Years 1 (0/150)

# Sac Regression: The Ultimate Indicator of EVAR Success

Not only sac expansion, but any failure for the sac to regress is associated with higher long-term mortality. 18


73% of patients with hostile neck anatomy.8 (27/37)


TREO consistently shows durable high Sac Regression and low sac expansion rates across multiple studies

## TREO Aneurysm sac changes @ 1 year and 5 years

	IDE <sup>1</sup> (1&5 years)	MARONE, et al <sup>8*</sup> (5 years)	Feasibility Study <sup>17</sup> (1&5 years)	RATIONALE* 4 (1 year)	US PAS <sup>^ 15</sup> (1 year)	EVAR VQI Multi Manuf. <sup>18</sup> (TREO not incl)(1 year)
	n=136	n=31	n=28	n=202	n=226	n=14,817
Decrease	46%	71%	54%	54%	46%	40%
Stable	54%	29%	46%	43%	50%	35%
Increase	0%	0%	0%	3%	4%	25%
Decrease @5 Years	<b>61%</b> 19 N=70	<b>71</b> %	<b>81%</b>			

<sup>^</sup> TREO US PAS is an all-comers study, follow-up on-going






### **EVAR Success: Sac Regression**


- ▶ 32% aneurysm size reduction (23mm) at 1 Year
- Without usage of adjunctive devices

## Long main body optimizes sac regression


\*\* The proximity of the distal end of the stent graft to the iliac bifurcation might promote sac regression, provide greater resistance to migration, and counter endograft shortening resulting from aortoiliac tortuosity. \*\*\*

# TREO Sizing

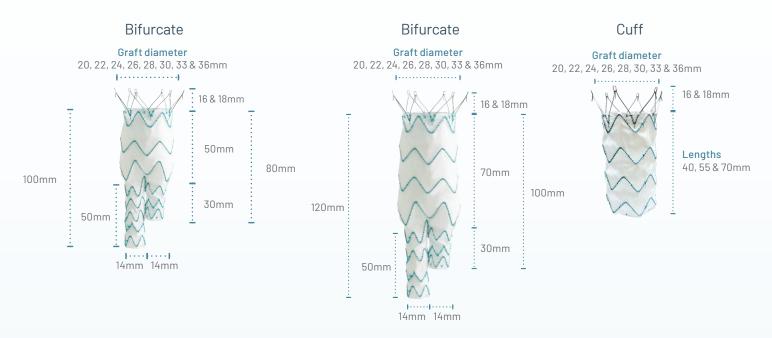

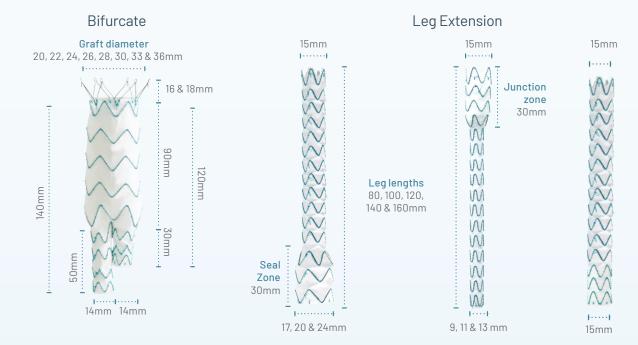

# TREO Product Ordering Information



## **Device Type Key**

B = Bifurcate L = Leg Extension C = Cuff S = Straight Extension

10

10

10

10

10

10

10

10

10

10

10

10

10

10

10

15

15

15

15

15

15

15

15

15

15

15

15

15

15

15

9

10-11

12-13

14-15

16-17

18-20

11

11

11

11

11

13

13

13

13

13

15

15

15

15

15

17

17

17

17

17

20

20

20

20

20

24

24

24

24

24

80

100

120

140

160

80

100

120

140

160

80

100

120

140

80

100

120

140

160

80

100

120

140

160

80

100

120

140

160

13 Fr

14 Fr

Catalog

Number

28-L2-09-080U

28-L2-09-100U

28-L2-09-120U

28-1 2-09-14011

28-L2-09-160U

28-L2-11-080U

28-L 2-11-100U

28-L2-11-120U

28-L2-11-140U

28-L2-11-160U

28-L 2-13-080U

28-L2-13-100U

28-L2-13-120U

28-L2-13-140U

28-L2-13-160U

28-L2-15-080U

28-L2-15-100U

28-L2-15-120U

28-L2-15-140U

28-L2-15-160U

28-L2-17-080U

28-L2-17-100U

28-L2-17-120U

28-L2-17-140U

28-L2-17-160U

28-L2-20-080U

28-L2-20-100U

28-L2-20-120U

28-L2-20-140U

28-L2-20-160U

28-L2-24-080U

28-L2-24-100U

28-L 2-24-120U

28-L2-24-140U

28-L2-24-160U

MTO<sup>1</sup>

## Main Body Bifurcate Stent-Graft

#### Leg Extension Stent-Graft Iliac Landing Aortic Outer Proximal Contralateral Profile Extension Zone MTO<sup>^</sup> Diameter Diameter Length OD Number Iliac Outer Minimum Distal Profile Covered Diameter Length Diameter Length OD 10 9 80 13 Fr 10 9 100 13 Fr 8 10 9 120 13 Fr 10 9 140 13 Fr 9 10 160 13 Fr

	20	80	18 Fr		28-B2-20-080U
17-18	20	100	18 Fr	•	28-B2-20-100U
	20	120	18 Fr	•	28-B2-20-120U
	22	80	18 Fr		28-B2-22-080U
18-19	22	100	18 Fr		28-B2-22-100U
	22	120	18 Fr	•	28-B2-22-120U
	24	80	18 Fr		28-B2-24-080U
19-21	24	100	18 Fr		28-B2-24-100U
	24	120	18 Fr	•	28-B2-24-120U
	26	80	18 Fr		28-B2-26-080U
21-23	26	100	18 Fr		28-B2-26-100U
	26	120	18 Fr		28-B2-26-120U
	28	80	18 Fr		28-B2-28-080U
23-25	28	100	18 Fr		28-B2-28-100U
	28	120	18 Fr		28-B2-28-120U
	30	80	19 Fr		28-B2-30-080U
25-27	30	100	19 Fr		28-B2-30-100U
	30	120	19 Fr		28-B2-30-120U
	33	80	19 Fr		28-B2-33-080U
27-30	33	100	19 Fr		28-B2-33-100U
	33	120	19 Fr		28-B2-33-120U
	36	80	19 Fr		28-B2-36-080U
30-32	36	100	19 Fr		28-B2-36-100U
	36	120	19 Fr		28-B2-36-120U

## Straight Extension Stent-Graft#

Iliac Outer Diameter	Iliac Landing Zone Minimum Length	Straight Extension Distal Diameter	Covered Length	Profile OD	Catalog Number
8	10	9	80	13 Fr	28-S2-09-080U
9	10	11	80	13 Fr	28-S2-11-080U
10-11	10	13	80	13 Fr	28-S2-13-080U

#### Distal iliac landing zone with:

- an inside diameter of 8mm 13mm and a length of ≥ 10mm or
- an inside diameter of >13mm 20mm and a length of ≥ 15mm

#### Proximal aortic landing zone with:

- Infrarenal landing neck length of ≥15mm
- Suprarenal neck angle of ≤ 45 degrees
- Infrarenal neck angle of ≤ 60 degrees
- Aortic neck diameters ≥17mm and ≤32mm
- # Straight Extension Stent-Grafts indicated for use only with previously implanted Leg Extension Stent-Grafts with the same distal diameter.
- ^ Made To Order devices are not kept in stock. They will be built upon receipt of Purchase Order and are subject to extended lead times.

# TREO Product Ordering Information

## Proximal Cuff Extension Stent-Graft

Aortic Outer Diameter	Proximal and Distal Diameter	Covered Length	Profile	MT0 <sup>^</sup>	Catalog Number
	20	40	18 Fr	•	28-C2-20-040U
17-18	20	55	18 Fr	•	28-C2-20-055U
	20	70	18 Fr		28-C2-20-070U
	22	40	18 Fr		28-C2-22-040U
18-19	22	55	18 Fr	•	28-C2-22-055U
	22	70	18 Fr		28-C2-22-070U
	24	40	18 Fr		28-C2-24-040U
19-21	24	55	18 Fr	•	28-C2-24-055U
	24	70	18 Fr		28-C2-24-070U
	26	40	18 Fr		28-C2-26-040U
21-23	26	55	18 Fr	•	28-C2-26-055U
	26	70	18 Fr		28-C2-26-070U
	28	40	18 Fr		28-C2-28-040U
23-25	28	55	18 Fr	•	28-C2-28-055U
	28	70	18 Fr		28-C2-28-070U
	30	40	19 Fr		28-C2-30-040U
25-27	30	55	19 Fr	•	28-C2-30-055U
	30	70	19 Fr		28-C2-30-070U
	33	40	19 Fr		28-C2-33-040U
27-30	33	55	19 Fr	•	28-C2-33-055U
	33	70	19 Fr		28-C2-33-070U
	36	40	19 Fr		28-C2-36-040U
30-32	36	55	19 Fr	•	28-C2-36-055U
	36	70	19 Fr		28-C2-36-070U

<sup>^</sup> Made To Order devices are not kept in stock. They will be built upon receipt of Purchase Order and are subject to extended lead times.



DISCOVER MORE Features and Benefits of TREO®

#### Features and Benefits:

#### terumoaortic.com/features-benefits

Discover how each of the key features and benefits are integrated into every one of our products to ensure the highest quality and performance possible.



DURABILITY & RELIABILITY











## References

- 1. Eagleton, M.J et al. "Safety and effectiveness of the TREO stent graft for the endovascular treatment of abdominal aortic aneurysms." Journal of Vascular Surgery vol. 74, 1(2021): pp.114–123. E3. doi.org/10.1016/j.jvs.2020.10.083.
- 2. TREO US IFU
- 3. Howell et al. "Computational fluid dynamics within bifurcated abdominal aortic stent-grafts." Journal of Endovascular Therapy vol. 14, 2 (2007): pp. 138-143. doi:10.1177/152660280701400204
- 4. Uberoi et al. "Global Post-Market Clinical Follow-up of the Treovance Stent-Graft for Endovascular Aneurysm Repair: One-Year Results From the RATIONALE Registry." Journal of Endovascular Therapy vol. 25, 6 (2018): pp. 726-734. doi:10.1177/1526602818803939
- Georgakarakos, E et al. "Computational estimation of the influence of the main body-to-iliac limb length ratio on the displacement forces acting on an aortic endograft; theoretical application to Bolton Treovance abdominal stent-graft." International Angiology vol. 33, 5 (2014): pp. 480-484.
- 6. Image courtesy of Dr. Heath Broussard.
- 7. Image courtesy of Dr. John Rollo.
- 8. Marone et al. "Five-Year Outcomes of Endovascular Aortic Repair With the TREO Abdominal Endograft." Journal of Endovascular Therapy vol. 0, 0 (2023). doi:10.1177/15266028231170161
- 9. Images courtesy of Dr. Tamer Boules.
- 10. Boitano et al. "The TREO abdominal aortic stent-graft system." Future Cardiology (2020). https://doi.org/10.2217/fca-20200158.
- 11. Terumo Aortic 2023 benchtop testing data on file.
- 12. Giannoni, M et al. "Contrast-Enhanced Ultrasound Imaging for Aortic Stent-Graft Surveillance." Journal of endovascular therapy vol. 10 (2003): pp. 208-217.
- 13. El Beyroutil, H. et al. "Early results of a low-profile stent-graft for thoracic endovascular aortic repair". PLoS One vol. 15, 11(2020): pp. e0240560.
- 14. Bi, G. "Is percutaneous access superior to cutdown access for endovascular abdominal aortic aneurysm repair? A meta-analysis". Vascular Vol. 30, 5 (2022): pp. 825–833.
- 15. Terumo Aortic TREO US Post Approval Study Report P190015 2023 data on file.
- 16. Case images courtesy of Dr. Beejay Feliciano.
- 17. Terumo Aortic TREO Annual Report 100200 2019 data on file.
- 18. O'Donnell, T et al. "Aneurysm sac failure to regress after endovascular aneurysm repair is associated with lower long-term survival." Journal of Vascular Surgery (2019): pp. 414-422. doi: 10.1016/j.jvs.2018.04.050.
- 19. Eagleton M, Stoner, M. TREO US IDE 5-year Data Presentation VEITH 2023.
- 20. Case images courtesy of Dr. Jonathon Rollo.

## Committed to Aortic Care



Discover solutions for every segment of the aorta terumoaortic.com







View IFU at eifu.terumoaortic.com for more information on use, indications, contraindications and warnings/precautions.

Product availability subject to local regulatory approval.

For distributor information, visit terumoaortic.com/contact

■ Bolton Medical Inc. 799 International Parkway, Sunrise, Florida 33325, USA