




SAFETY & EFFICACY



# RELAY<sup>®</sup> PRO

THORACIC STENT-GRAFT SYSTEM

Uniquely Inspired  
for Ideal Placement

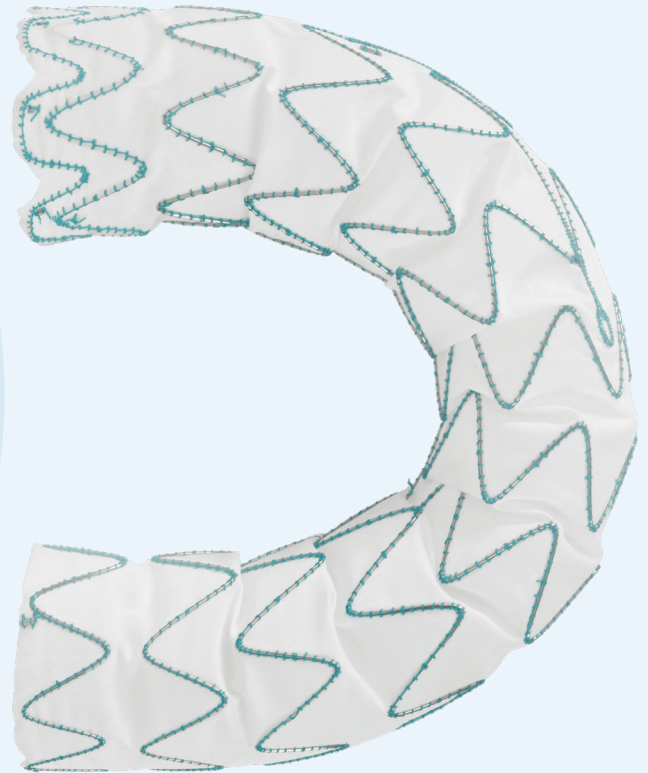


For more information, visit  
[terumo.com/features-benefits](https://www.terumo.com/features-benefits)

**TERUMO**  
AORTIC

# Navigating the Arch with Care with Dual Sheath Technology

An integrated **Dual Sheath** system which **minimizes access vessel manipulation** and **provides atraumatic** thoracic aorta **navigation**:

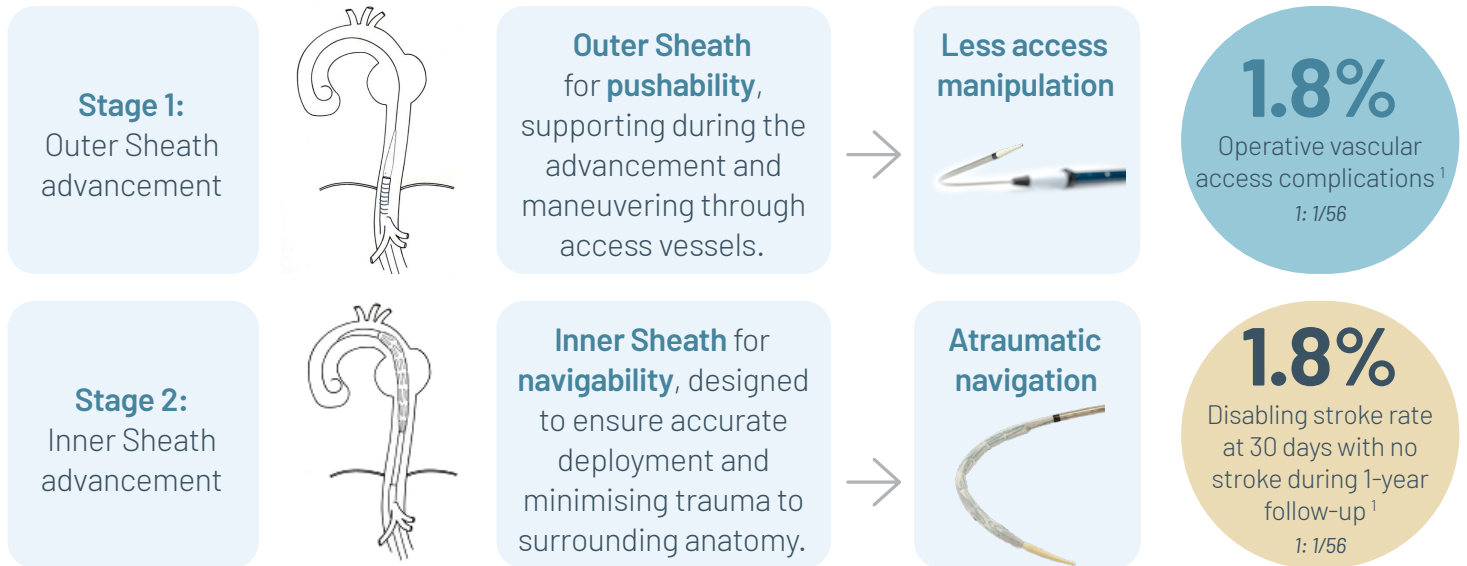

1: Acute complicated Type B aortic Dissection Cohort

*“Relay®Pro’s ability to navigate smoothly over the arch as a result of the Dual Sheath system enables accurate deployment, and combined with the low profile of the device, this allows me to successfully treat complex anatomy with precision.”<sup>2</sup>*



WATCH ON VUMEDI

How to minimize air embolisms during thoracic endovascular aortic repair with Relay®Pro?

1. Rossi, P.J et al. 2023. One-Year Results of a Low-Profile Endograft in Acute, Complicated Type B Aortic Dissection. *The Annals of Thoracic Surgery*.

2. Wilson Y. Szeto, MD. Chief, Division of Cardiovascular Surgery. Hospital of the University of Pennsylvania-Penn Presbyterian - [www.temmo.com/newsrelease/detail/20210806/634](http://www.temmo.com/newsrelease/detail/20210806/634)

# Uniform Sealing and Secure Fixation with Proximal End Configuration

Relay<sup>®</sup>Pro comes in two proximal stent configurations: bare stent and non-bare stent (NBS):

## BARE STENT CONFIGURATION

**Partial overlapping** of the bare stent with the first covered stent to **maximize** the number of **sealing points**.


## NON BARE STENT CONFIGURATION

A crown-shaped nitinol stent overlapping with the proximal sealing stent, both covered with fabric, designed to maximize conformability and **minimize infolding**.

## HIGH RADIAL LOAD

Both proximal configurations are designed to deliver **high radial load** for an effective apposition and fixation of the graft against the aortic wall.


## Multiple Sealing Points



**1.8%**

Type Ia endoleak at 12 months <sup>1,3</sup>


1: 1/56  
3: 2/110



**100%**

Technical success through 24 hours <sup>1,3</sup>

1: 56/56  
3: 110/110

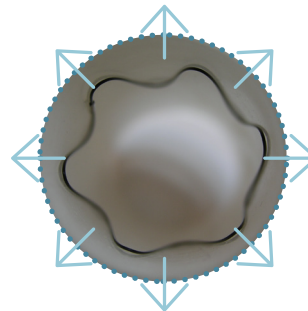

**0%**

Migration through 12 months <sup>3</sup>

3: 0/110

1: Acute Complicated Type B Aortic Dissection Cohort

3: Thoracic Aortic Aneurysm and Penetrating Atherosclerotic Ulcer Cohort

1. Rossi, P.J et al. 2023. One-Year Results of a Low-Profile Endograft in Acute, Complicated Type B Aortic Dissection. *The Annals of Thoracic Surgery*.

3. Szeto et al. 2022. One-Year Results with a Low-Profile Endograft in Subjects with Thoracic Aortic Aneurysm and Ulcer Pathologies. *The Journal of Thoracic and Cardiovascular Surgery*



Discover solutions for every segment of the aorta  
[terumoortic.com](https://www.terumoortic.com)



LinkedIn



VuMedi



X