




TREO® ABDOMINAL STENT-GRAFT SYSTEM

Versatile by Design. Fit for any Anatomy.*


*Per IFU.

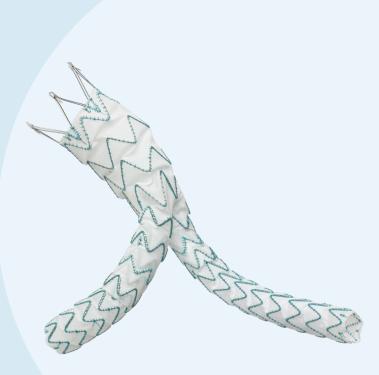



For more information, visit terumoaortic.com/features-benefits

More Choices, More Possibilities Multiple size options for planning and treatment

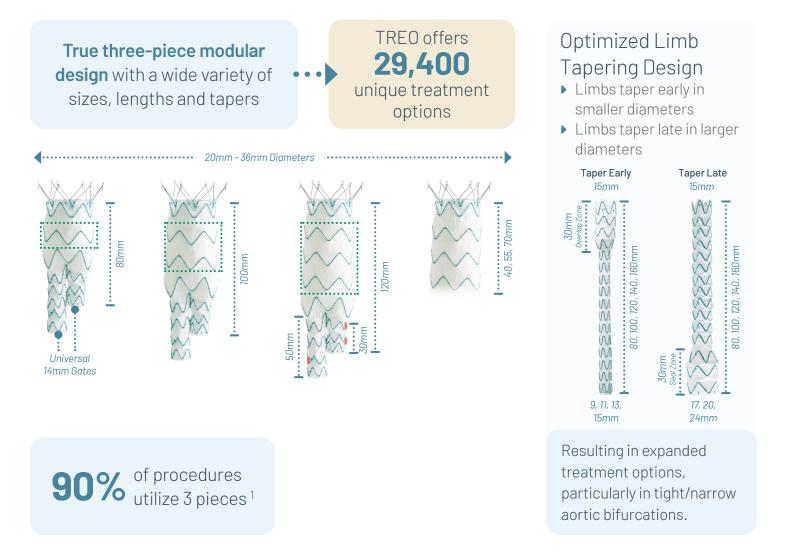

1. TREO IFU

Howell BA, Kim T, Cheer A, Dwyer H, Saloner D, Chuter TAM. Computational fluid dynamics within bifurcated abdominal aortic stent-grafts. J Endovasc Ther. 2007;14(2):138-143. doi:10.1177/152660280701400204
Uberoi R, Setacci C, Lescan M, et al. Global Post-Market Clinical Follow-up of the Treovance Stent-Graft for Endovascular Aneurysm Repair: One-Year Results From the RATIONALE Registry. J Endovasc Ther. 2018;25(6):726-734. doi:10.1177/1/52660280701400204







Provides the ideal platform for both present and future EVAR needs

Long main bodies provide:

- ▶ Lower displacement forces and increased endograft stability during the cardiac cycle ^{2, 4}
- Endograft closer to aortoiliac bifurcation makes it easier and faster to cannulate contralateral gate ³

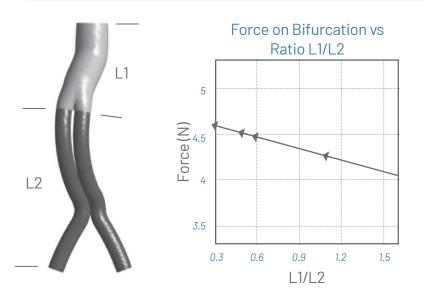

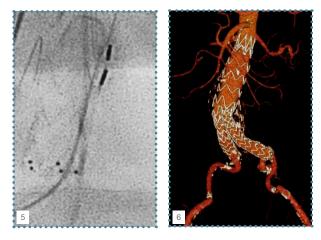

Ease of gate cannulation with long main body

TREO's long main body's ability to sit close to aortoiliac bifurcation, along with limb lock mechanism, may reduce the risk of both proximal and distal migration. ⁴

- 4. Georgakarakos E, Xenakis A, Georgiadis GS, et al. Computational estimation of the influence of the main body-to-iliac limb length ratio on the displacement forces acting on an aortic endograft. Theoretical application to Bolton Treovance® Abdomina
- 5. Image courtesy of Dr. Heath Broussard
- 6. Image on file; courtesy Dr. John Rollo





Discover solutions for every segment of the aorta terumoaortic.com





View IFU at eifu.terumoaortic.com for more information on use, indications, contraindications and warnings/precautions.

Product availability subject to local regulatory approval.

Bolton Medical Inc. 799 International Parkway, Sunrise, FL 33325, United States

